

MINIMUM INSTALLATION REQUIREMENTS VARY DEPENDING ON SENSOR DENSITY, cont'd.

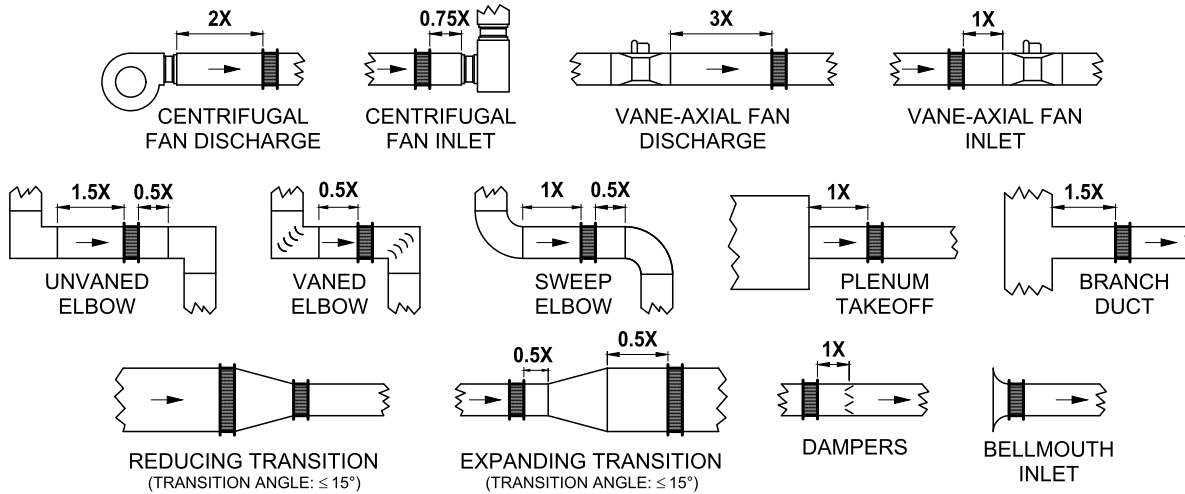


Figure 1

ELECTRA-flo/S5 Probe Array (Level 1), ELECTRA-flo/S5-MM Station (Level 1), ELECTRA-flo/S5-CM Station (Level 2)

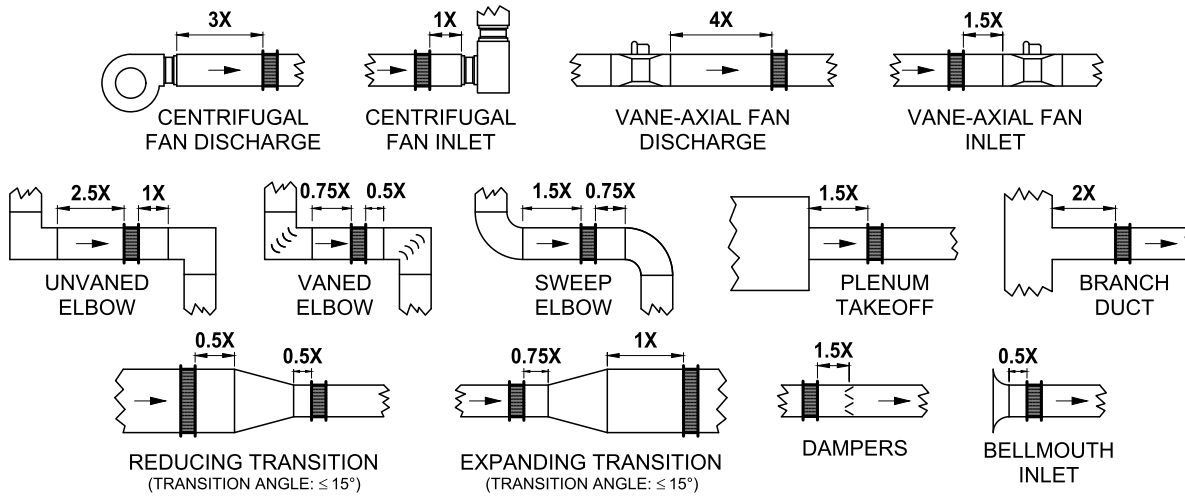


Figure 2

ELECTRA-flo/S5 Probe Array (Level 2), ELECTRA-flo/S5-MM Station (Level 2), ELECTRA-flo/S5-CM Station (Level 3)

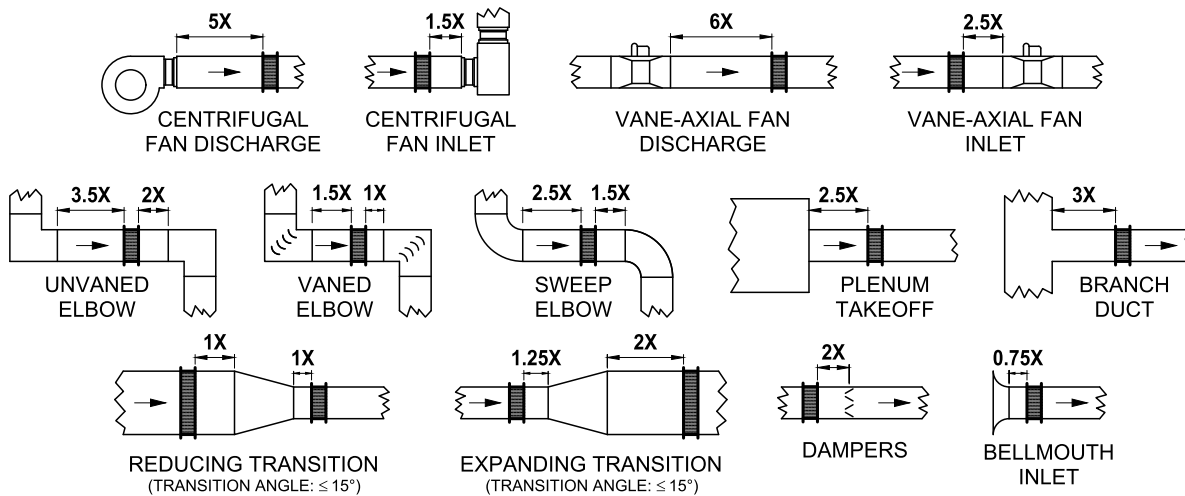


Figure 3

ELECTRA-flo/S5 Probe Array (Level 3) & ELECTRA-flo/S5-MM Station (Level 3)